

FIG.1

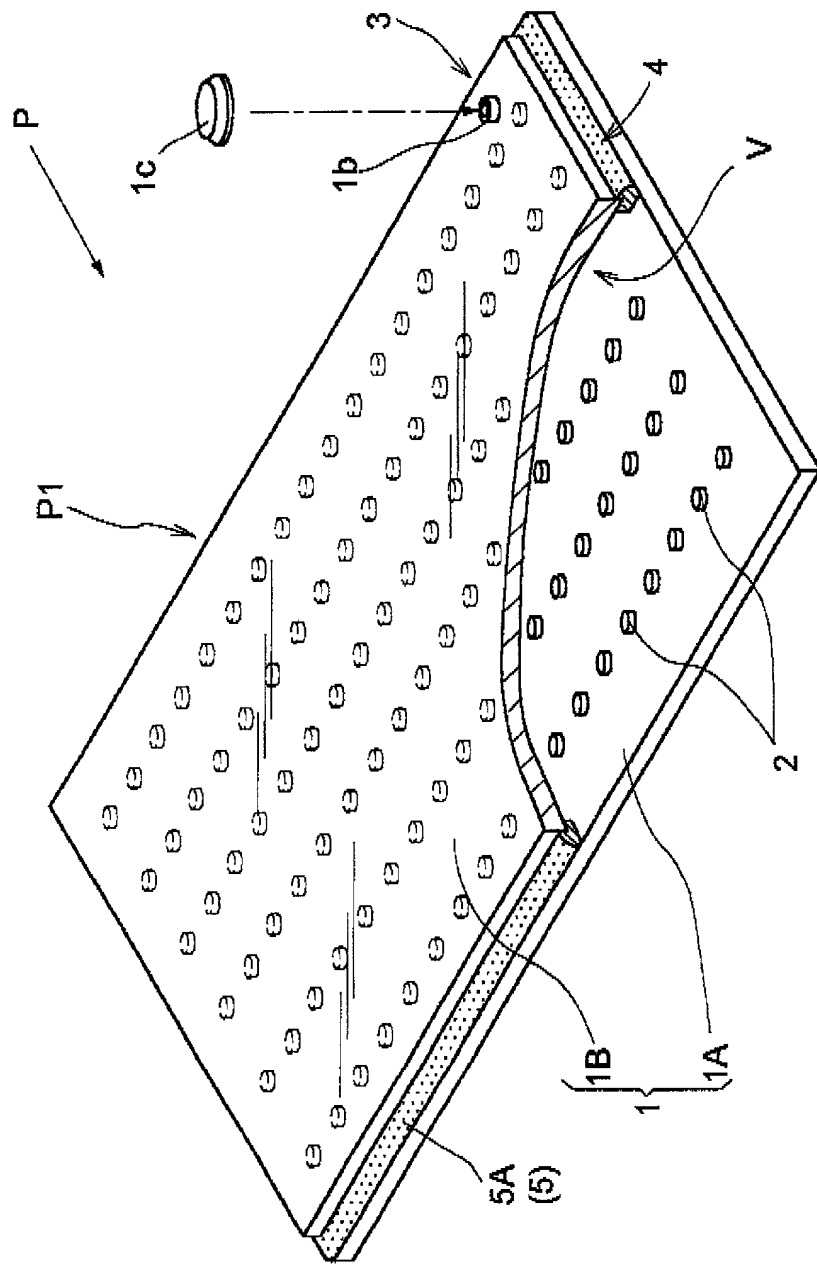
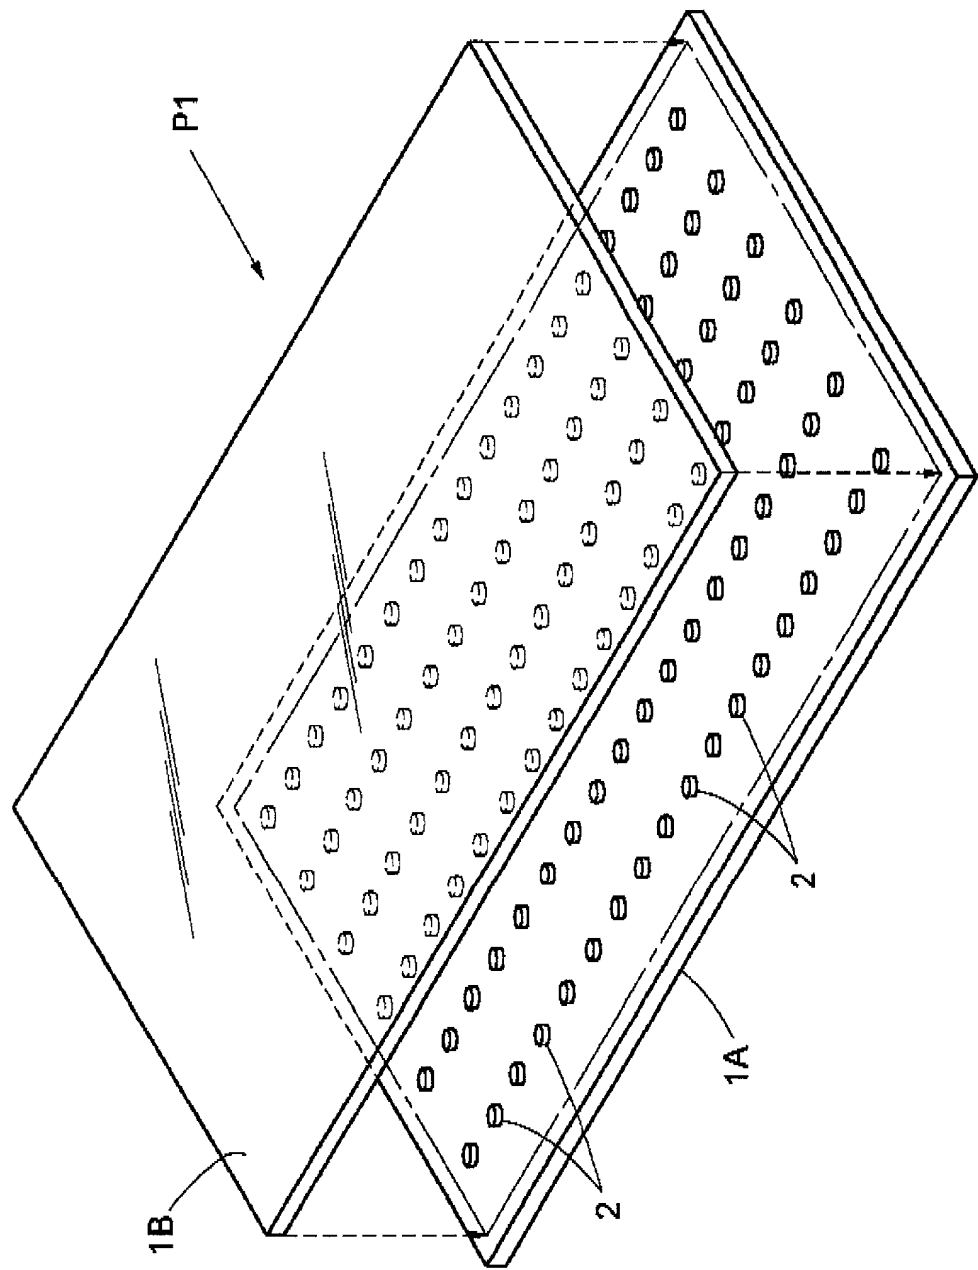


FIG. 3



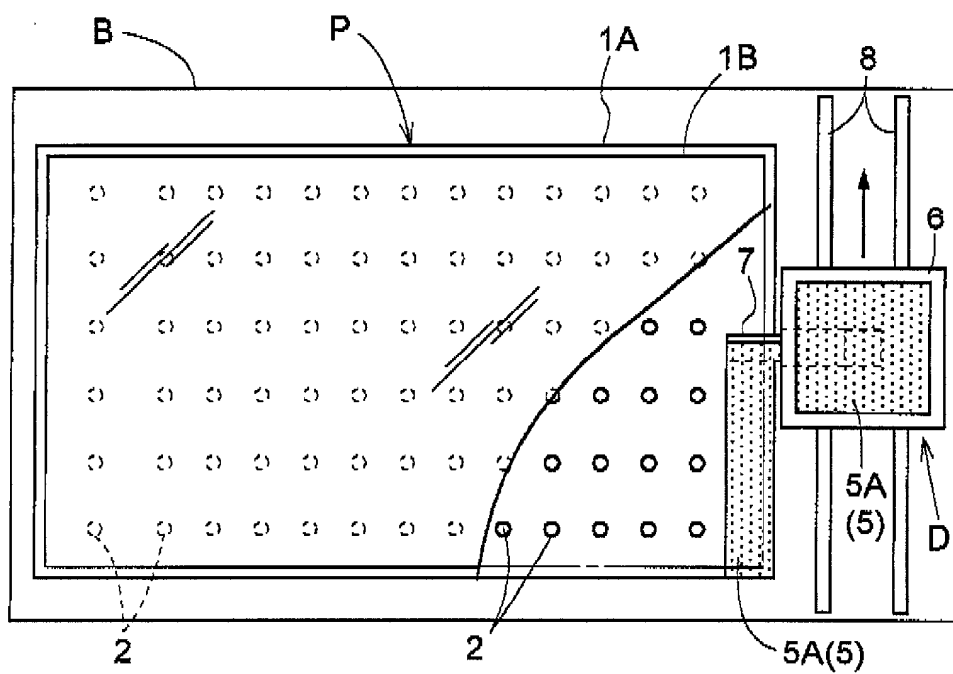


FIG.6

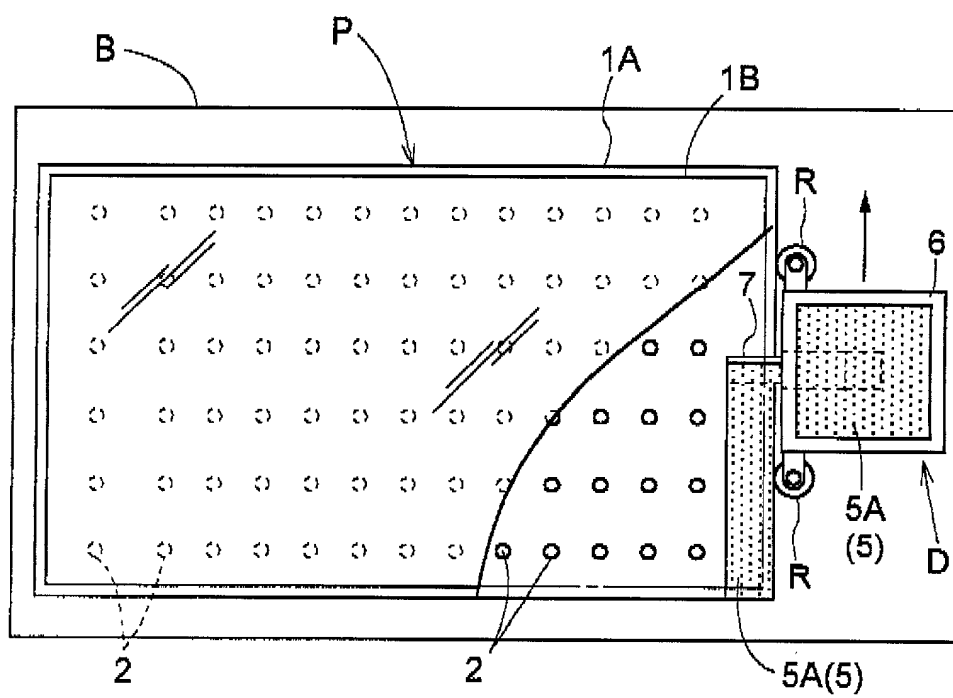


FIG. 7

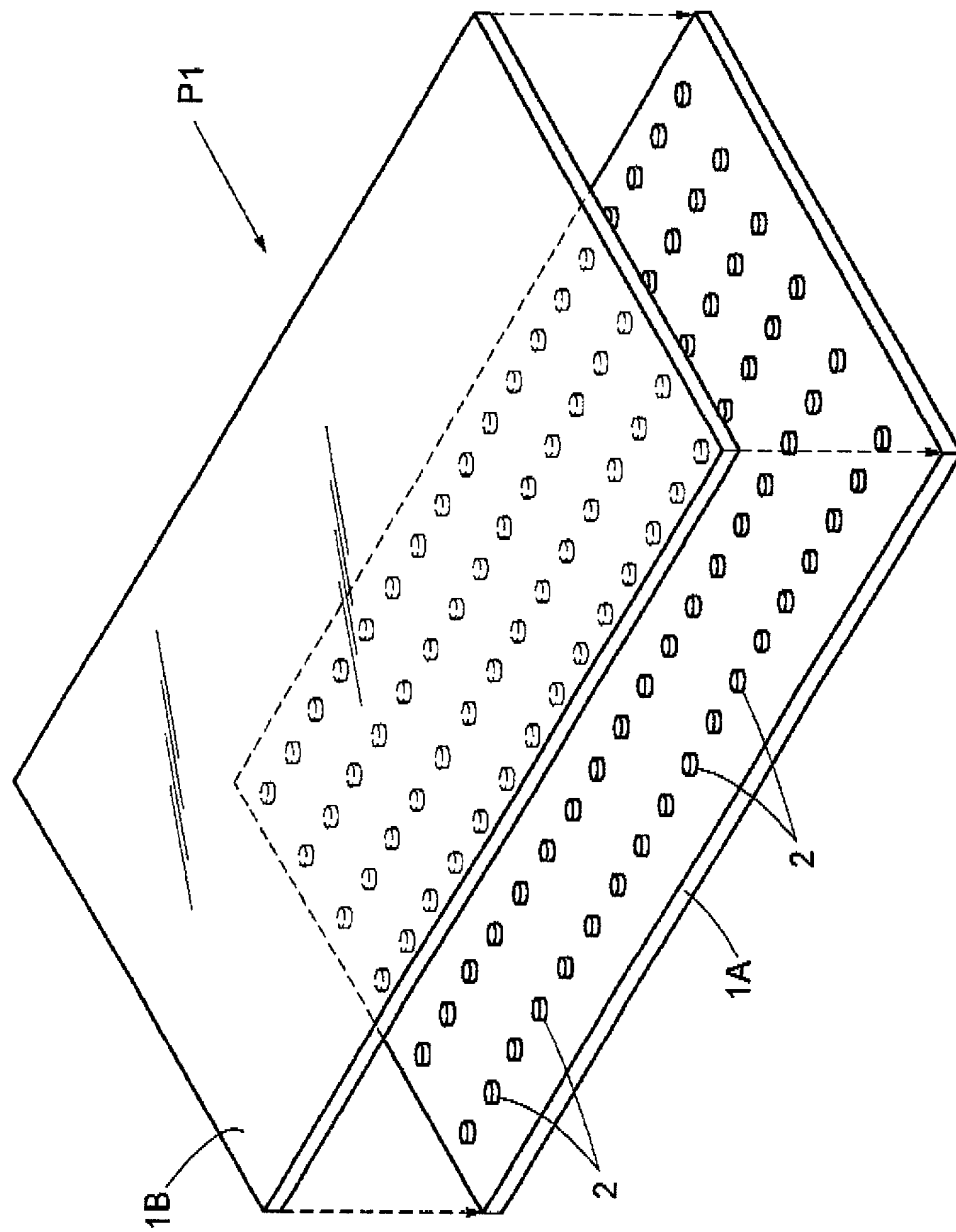


FIG.8

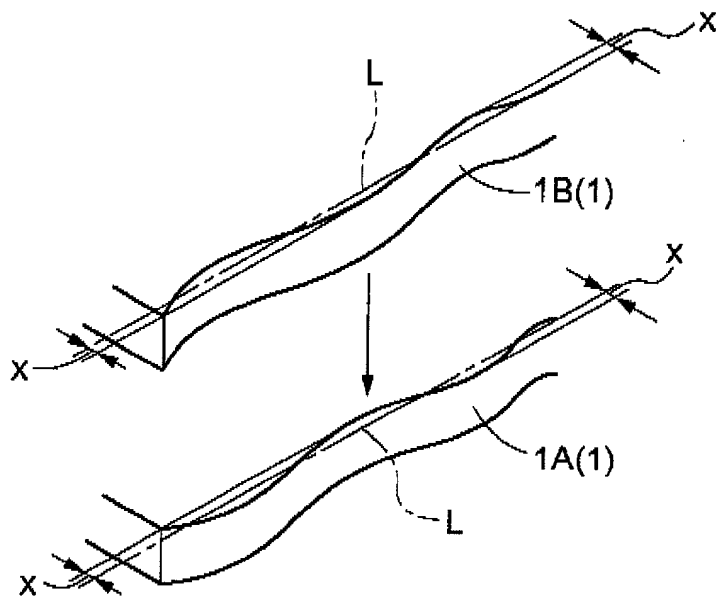


FIG.9

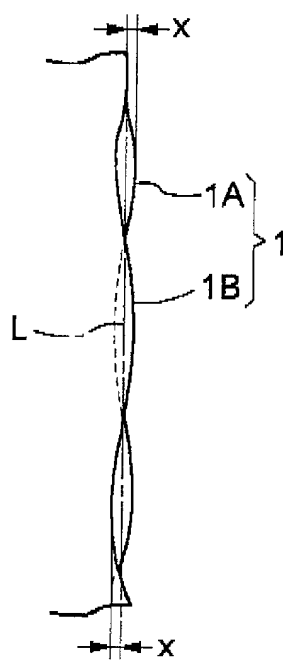


FIG.10

| Sample No. | Projection amount (mm) | Sealing result |
|------------|------------------------|----------------|
| 1 | 0 | good |
| 2 | +2.5 | no good |
| 3 | -4.0 | no good |
| 4 | -2.0 | good |
| 5 | -1.0 | good |

FIG.11

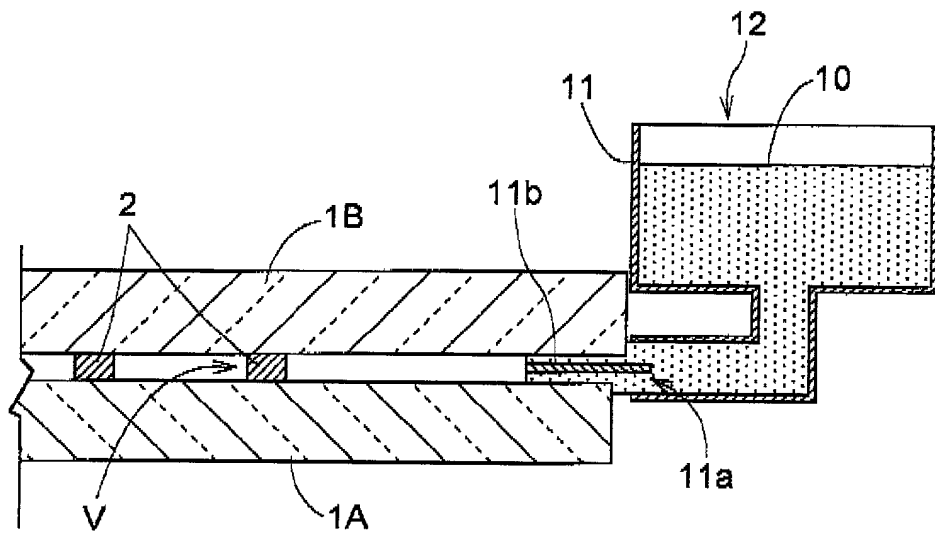


FIG.12

